Negotiated Comparison

BBMP/2021-22/OW/WORK_INDENT47270/CALL-2

Grants of Infrastructure up gradation of Yelahanka Govt Hospital

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
1	VVIP Excecutive Chair – : Fire retardant breathable mesh for backrest and Polyester fabric for seat. Black colour on seat and back (TW 182 Mesh & 5060 fabric seat) Base : 700 mm diameter raised Nylon base with 60 mm castors for stability and easy movement . Seat cover : Casement cloth protection for seat understructure Adjustable Arms : Moves up or down for shoulder and upper body support. The firm polyurethane arm pads adjust vertically to accommodate different arm lengths from the shoulder to the elbow (TSA012 – value lab pad) Lumbar Support: "S' shaped backrest follow's the natural curve of the back for lower back support. Additional support by static polypropylene lumbar pad on back rest . Seat Contour : Seat pan depth is designed so that the forward most point on the lumbar support is placing gentle pressure on the lower 5 vertebrae on the spine. (2018 – Nuclear Seat) Synchro tilt with single lock : Chair Back reclines synchronously to a 2-to-1 ratio to seat angle. Allows user to recline while keeping seat cushion relatively level to floor. Use the tilt lock for upright posture like keyboarding . Pneumatic height : Change the height of the chair relative to the floor by 100 mm . Headrest : Fixed head rest for neck support	NO	3.00	11800.00	35400.00	12608.00	37824.00	12381.06	37143.17
2	Doctor's Executive Chair : 1. High back chair with head support. 2. The double mesh back should be designed for comfort and support. 3. Adjustable seat height, head rest height & Hand rest angle 4. Adjust the height using the gas lift to find that comfortable position, and the nylon castors make it easy to move around your space. 5. Five-part Chrome legs 6. Height 48" + 2" 7. Width 26" + 2" 8. Depth 20" + 2" Should be ISI / CE certified	NO	10.00	8850.00	88500.00	9456.00	94560.00	9285.79	92857.92
3	Cardiac Cots: 1.◆ Laminated board Top.◆ 2.◆ Tubular steel frame work.◆ 3.◆ Mounted on four 5cm. castors.◆ 4.◆ Epoxy powder coated.◆ 5.◆ Top size: -106(L)*45(W) cm.Height: -95cm	NO	6.00	3540.00	21240.00	3782.00	22692.00	3713.92	22283.54
4	Steel Racks: 1. Steel rack made of slotted angles of size 2"x2"x3mm thick, 2. 5 compartments of six 6' x 1 ¼'x 3' length. 3. Paint: Epoxy powder coated in seamen's Gray Colour with minimum 50 microns 4. Should be ISI / CE Certified	NO	12.00	5900.00	70800.00	6304.00	75648.00	6190.53	74286.34
5	Patient Cots (Plain):1. Size-78"Lx36"Wx24"H, 1 ¼" dia 14 SWG tubular Head and leg bows ERW Tube.2. The head bow and leg bows are 42" and 36" Height respectively. Head and leg bows are 14 gauge, 1" dia ERW cross bar and ½" dia 16-gauge ERW three vertical support bars.3. Top Sheet 18 SWG CRCA Sheet, double Press bent uniformly on all the four sides, 2" vertically and ¾" further inside. A 6" broad x 2" deep full length 16-gauge square cross section rib is reinforced to the top sheet 2 Nos. M.S. Gages using 10 SWG. 4. Zinc plated ½" nuts & bolts, 4 Nos. of Shoes made up of white nylon are provided. 5. Epoxy powder coated with seamen's Gray Colour with 50 microns minimum coating.	NO	10.00	5900.00	59000.00	6304.00	63040.00	6190.53	61905.28

123810.56

Scanned by TapScanner

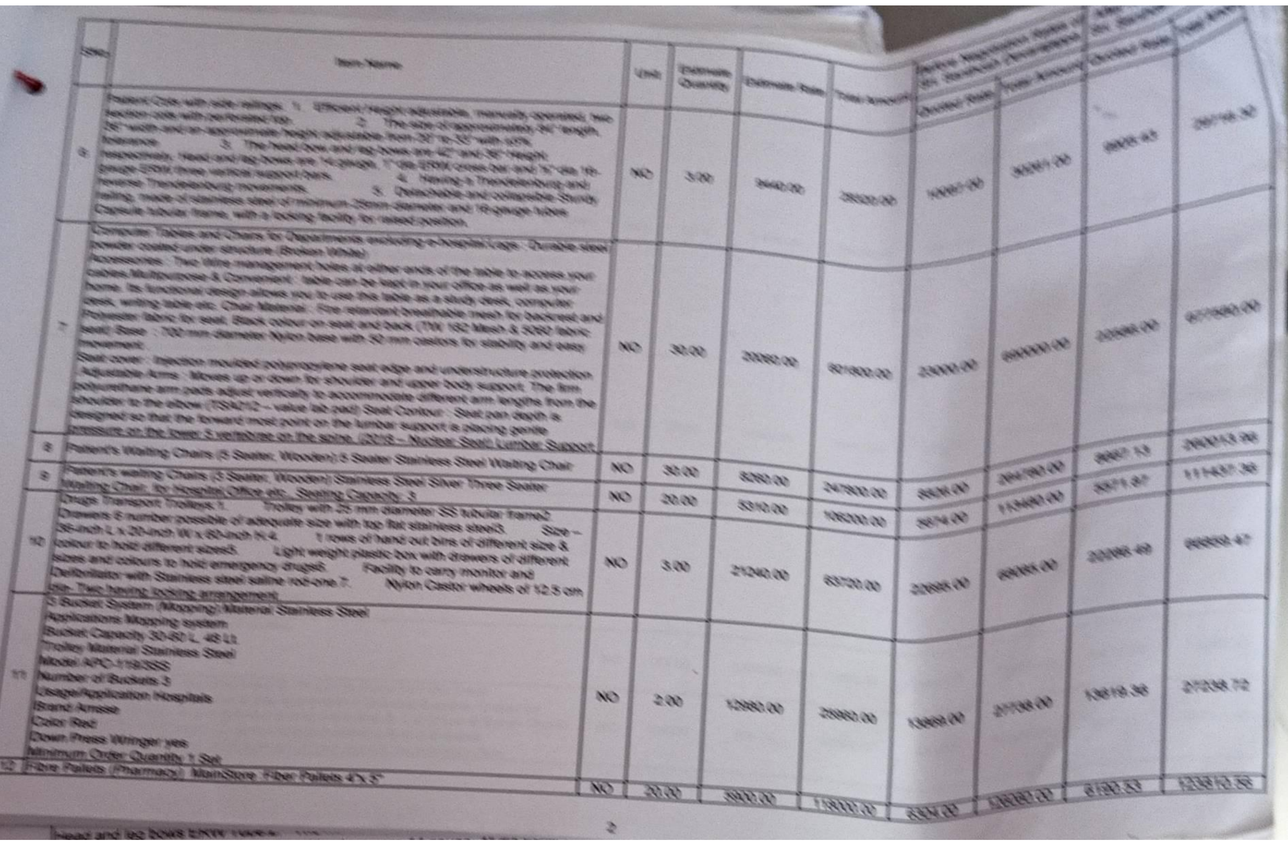

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Approx Manufacturers Market rate inc. Transport, Unloading etc.		After Discount	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
6	Patient Cots with side railings: 1. Efficient / Height adjustable, manually operated, two section cots with perforated top. 2. The size of approximately 76" length, 36" width and an approximate height adjustable from 22" to 32" with 10% tolerance. 3. The head box and leg boxes are 42" and 56" Height, respectively. Head and leg boxes are 14-gauge, 1" dia (OD) cross bar and ¼" dia 16-gauge (OD) three vertical support bars. 4. Having a Trendelenburg and reverse Trendelenburg movements. 5. Detachable and collapsible Sturdy, resting, made of stainless steel of minimum 24mm diameter and 16-gauge tubes. Capsule tubular frame, with a locking facility for raised position.	NO	3.00	9442.00	28326.00	10661.00	31983.00	8906.45	26716.32
7	Computer Tables and Chairs for Departments excluding e-hospital Legs : Durable steel powder coated under structure (Broken White) Accessories : Two Wire management holes at either ends of the table to access your cables.Multipurpose & Convenient : table can be kept in your office as well as your home. Its functional design allows you to use this table as a study desk, computer desk, writing table etc. Chair Material : Fire retardant breathable mesh for backrest and Polyester fabric for seat, Black colour on seat and back (TW 182 Mesh & 5260 fabric) Seat: Base : 700 mm diameter Nylon base with 50 mm castors for stability and easy movement. Seat cover : Injection moulded polypropylene seat edge and understructure protection. Adjustable Arms : Moves up or down for shoulder and upper body support. The firm polyurethane arm pads adjust vertically to accommodate different arm lengths from the shoulder to the elbow (TSA212 – value tab pad) Seat Contour : Seat pan depth is designed so that the forward most point on the lumber support is placing gentle pressure on the lower 5 vertebrae on the spine. (2016 – Nucleus Seat) Lumbar Support	NO	30.00	20980.00	621900.00	23000.00	690000.00	20986.00	629580.00
8	Patient's Waiting Chairs (5 Seater, Wooden) 5 Seater Stainless Steel Waiting Chair	NO	30.00	8260.00	247800.00	8826.00	264780.00	8667.13	260013.90
9	Patient's waiting Chairs (3 Seater, Wooden) Stainless Steel Silver Three Seater Waiting Chair, for Hospital, Office etc., Seating Capacity: 3	NO	20.00	5310.00	106200.00	5674.00	113480.00	5571.67	111433.38
10	Drugs Transport Trolleys:1. Trolley with 25 mm diameter SS tubular frame2. Drawers 6 number possible of adequate size with top flat stainless steel3. Size – 36-inch L x 20-inch W x 60-inch H.4. 1 rows of hand out bins of different size & colour to hold different sizes5. Light weight plastic box with drawers of different sizes and colours to hold emergency drugs6. Facility to carry monitor and Defibrillator with Stainless steel saline rod-one 7. Nylon Castor wheels of 12.5 cm dia. Two having locking arrangement.	NO	3.00	21240.00	63720.00	22695.00	68085.00	22986.49	68959.47
11	5 Bucket System (Mopping) Material: Stainless Steel Applications Mopping system, Bucket Capacity 30-60 L, 46 Ltr, Trolley Material: Stainless Steel Model: APC-1193SS Number of Buckets: 5 Usage/Application: Hospitals Brand: Amese Color: Red Down Press Wringer: yes Minimum Order Quantity: 1 Set	NO	2.00	10980.00	21960.00	13669.00	27338.00	13616.36	27232.72
12	Fibre Pallets (Pharmacy) MainStore: Fiber Pallets 4'x 3"	NO	20.00	5900.00	118000.00	6534.00	130680.00	6197.53	123950.56

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
13	Dispensing Chairs:Material: Fire retardant breathable mesh for backrest and Polyester fabric for seat. Black colour on seat and back (TW 182 Mesh & 5060 fabric seat) Base : 700 mm diameter raised Nylon base with 60 mm castors for stability and easy movement . Seat cover : Casement cloth protection for seat understructure Adjustable Arms : Moves up or down for shoulder and upper body support. The firm polyurethane arm pads adjust vertically to accommodate different arm lengths from the shoulder to the elbow (TSA012 – value lab pad) Lumbar Support: "S' shaped backrest follow's the natural curve of the back for lower back support. Additional support by static polypropylene lumbar pad on back rest . Seat Contour : Seat pan depth is designed so that the forward most point on the lumbar support is placing gentle pressure on the lower 5 vertebrae on the spine. (2018 – Nuclear Seat) Synchro tilt with single lock : Chair Back reclines synchronously to a 2-to-1 ratio to seat angle. Allows user to recline while keeping seat cushion relatively level to floor. Use the tilt lock for upright posture like keyboarding .Pneumatic height : Change the height of the chair relative to the floor by 100 mm . Headrest : Fixed head rest for neck support	NO	3.00	11800.00	35400.00	12608.00	37824.00	12381.06	37143.17
14	Cushion Chair with Arm:Brand Maruthi Color option available Seat Material Fabric Size standard Design Type Customized No Of Wheels 5 Revolving Chair Yes Material cushion Condition New Minimum Order Quantity 1 Piece	NO	20.00	3540.00	70800.00	3782.00	75640.00	3713.92	74278.48
15	Blood Drawing Chair:Color Blue Material Stainless steel General Use Blood banks Brand Agile Number Of Seats 1 Weight 120 kg Automation Grade Remote Controlled Usage/Application Hospitals,Blood Banks Voltage 230 V	NO	2.00	76700.00	153400.00	81954.00	163908.00	80478.83	160957.66
16	Wooden Stool:Surface Finish Polished Material Wooden Shape Square Feature Termite Free	NO	30.00	2360.00	70800.00	2522.00	75660.00	2476.60	74298.12
17	Plastic Chair:◆◆◆ 1.◆◆◆◆◆◆◆◆◆ Should be made from the finest polypropylene.◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆ 2.◆◆◆◆◆◆◆◆◆ Should be Tough and lightweight.◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆ 3.◆◆◆◆◆◆◆◆◆ Should be Good quality and Modern designed.◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆ 4.◆◆◆◆◆◆◆◆◆ Should be Weatherproof and virtually maintenance free.	NO	100.00	826.00	82600.00	883.00	88300.00	867.11	86710.60

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
18	Wooden Tables with Drawers:Surface Finish PolishedMaterial Particleboard Size 4x2 Feet Shape Rectangular Warranty 1 Year Seating Capacity 1 Seater	NO	20.00	6844.00	136880.00	7313.00	146260.00	7181.37	143627.32
19	Wooden Almaraha With Glass Doors casuality to keep registers	NO	10.00	23600.00	236000.00	25217.00	252170.00	24763.09	247630.94
20	Sterile Equipments /bins Storage Trolly:Capacity 300 kg Brand Jindal Material Mild Steel	NO	5.00	5310.00	26550.00	5674.00	28370.00	5571.87	27859.34
21	Folding Cots:Material: Steel Pipe Capacity: 120 kg	NO	10.00	9440.00	94400.00	10087.00	100870.00	9905.43	99054.34
22	Almariha Steel:1. Size: 78" x 36" x 19" with 3 Shelves to be fixed having 4 compartments, 2. 1 compartment with Locker having lever lock placed in a suitable place. The locking system must be mounted securely to give robustness and long life. 3. Double door with three way locking device with duplicate keys, made out of CRCA Sheet of 18 gauge with de rusted synthetic enamel Siemens Gray colour paint. 4. The edges of doors and shelves should be properly bent to U Shape neatly and finished.	NO	5.00	12980.00	64900.00	13869.00	69345.00	13619.36	68096.79
23	Hospital Surrondings Dust Bins:RC Ventures Plastic Wheeled Dust Bin for Outdoor Usage/Application Outdoor Brand RC Ventures Material Plastic Capacity 120 Liters Number Of Wheels 2	NO	6.00	3540.00	21240.00	3782.00	22692.00	3713.92	22283.54
24	Wheel Barrows:Model Name/Number RJTE 005 Load Capacity 300 ltrs	NO	5.00	29500.00	147500.00	31521.00	157605.00	30953.62	154768.11
25	Stretcher: 1. Overall Size: Length 84". Width 24". Height 32" 2. Design Removable stretcher top made up of S.S. 20 SWG 304 Grade with full polish with removable cushion made up of 2" foam with inner cloth cover and S.T. quality Green Drill back rexine. 3. The top should be dished to a depth of not less than 1" not more than 2", further fixed on 1" diameter 18 SWG S.S. tubular frames. 4 legs. of 1" diameter 18 SWG supporting floor studs also to be provided, at the bottom of stretcher supporting frame of stretcher. Stretcher handle S.S. 18 SWG 304 grade round shape with full polish. 6" diameter 4 nos. swivelling castor rubber wheels 4. Should have with nylon shoes. 1.1/4" Sq. 16 SWG ER W pipes used for vertical and horizontal suitable stand for B-Type oxygen cylinder. 5. Epoxy powder coating in seamen's grey colour with minimum 50 microns. 6. Should be ISI / CE Certified.	NO	5.00	14160.00	70800.00	15130.00	75650.00	14857.66	74288.30
26	Wheel Chair:◆◆◆◆◆◆ 1.◆◆◆◆◆◆◆◆◆ Floor to seat height:650 mm to 720 mm.◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆ 2.◆◆◆◆◆◆◆◆◆ Overall Size Width:1000 mm to 1100 mm. Length 910 mm to 950 mm. Height 480 mm to 510 mm.◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆◆ 3.◆◆◆◆◆◆◆◆◆ Design: 1" Diameter 16 SWG ERW tubular frame fitted with metal seat and back. Adjustable horizontal aluminium foot rest 90◆ - 120◆ with tread flats. Half round Wooden Hand rest with 1" cushion. Solid rubber tyre wheels 24" x 1 W" fitted with self-propelling hoops and brake arrangement. Full length axle should be provided to fix the rickshaw wheel.	NO	5.00	5900.00	29500.00	6304.00	31520.00	6190.53	30952.64

Head and leg bows ERW Tube.2. The head bow and leg bows are
and 36" Height respectively. Head and leg bows are 14 gauge, 1" dia ERW
cross bar and ¼" dia 16-gauge ERW three vertical support bars 3. Top

Scanned by TapScanner

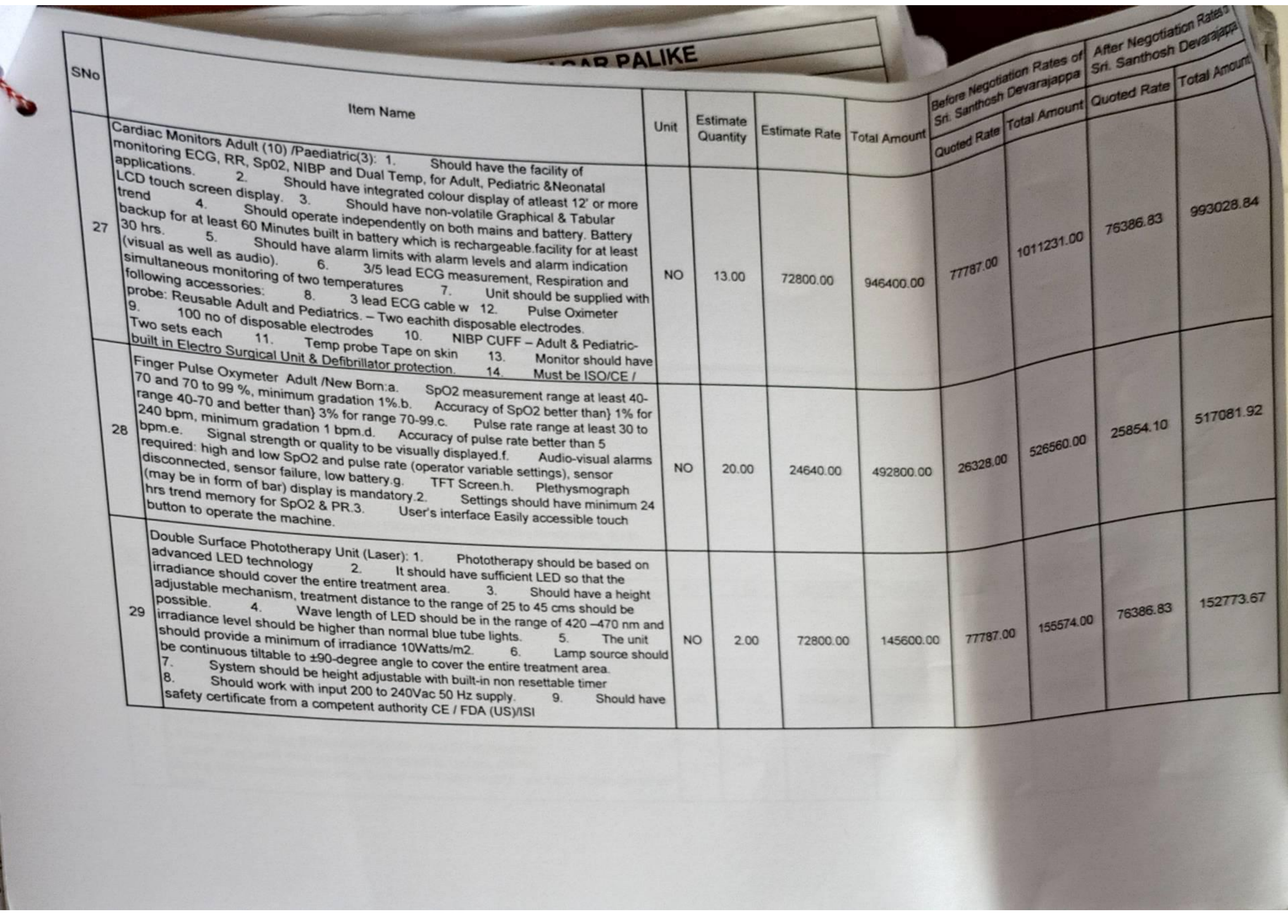

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
27	Cardiac Monitors Adult (10) /Paediatric(3): 1. Should have the facility of monitoring ECG, RR, Sp02, NIBP and Dual Temp, for Adult, Pediatric &Neonatal applications. 2. Should have integrated colour display of atleast 12' or more LCD touch screen display. 3. Should have non-volatile Graphical & Tabular trend. 4. Should operate independently on both mains and battery. Battery backup for at least 60 Minutes built in battery which is rechargeable facility for at least 30 hrs. 5. Should have alarm limits with alarm levels and alarm indication (visual as well as audio). 6. 3/5 lead ECG measurement, Respiration and simultaneous monitoring of two temperatures 7. Unit should be supplied with following accessories: 8. 3 lead ECG cable w 12. Pulse Oximeter probe: Reusable Adult and Pediatrics. – Two eachith disposable electrodes. 9. 100 no of disposable electrodes 10. NIBP CUFF – Adult & Pediatric-Two sets each 11. Temp probe Tape on skin 13. Monitor should have built in Electro Surgical Unit & Defibrillator protection. 14. Must be ISO/CE /	NO	13.00	72800.00	946400.00	77787.00	1011231.00	76386.83	993028.84
28	Finger Pulse Oxymeter Adult /New Born:a. SpO2 measurement range at least 40-70 and 70 to 99 %, minimum gradation 1%.b. Accuracy of SpO2 better than} 1% for range 40-70 and better than} 3% for range 70-99.c. Pulse rate range at least 30 to 240 bpm, minimum gradation 1 bpm.d. Accuracy of pulse rate better than 5 bpm.e. Signal strength or quality to be visually displayed.f. Audio-visual alarms required: high and low SpO2 and pulse rate (operator variable settings), sensor disconnected, sensor failure, low battery.g. TFT Screen.h. Plethysmograph (may be in form of bar) display is mandatory.2. Settings should have minimum 24 hrs trend memory for SpO2 & PR.3. User's interface Easily accessible touch button to operate the machine.	NO	20.00	24640.00	492800.00	26328.00	526560.00	25854.10	517081.92
29	Double Surface Phototherapy Unit (Laser): 1. Phototherapy should be based on advanced LED technology 2. It should have sufficient LED so that the irradiance should cover the entire treatment area. 3. Should have a height adjustable mechanism, treatment distance to the range of 25 to 45 cms should be possible. 4. Wave length of LED should be in the range of 420 –470 nm and irradiance level should be higher than normal blue tube lights. 5. The unit should provide a minimum of irradiance 10Watts/m2. 6. Lamp source should be continuous tiltable to ±90-degree angle to cover the entire treatment area. 7. System should be height adjustable with built-in non resettable timer 8. Should work with input 200 to 240Vac 50 Hz supply. 9. Should have safety certificate from a competent authority CE / FDA (US)/ISI	NO	2.00	72800.00	145600.00	77787.00	155574.00	76386.83	152773.67

Scanned by TapScanner

...NAGAR PALIKE

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
30	Electric Suction Apparatus, 1HP (3) /1/2 (6)HP new Born: 1. Should be a complete stainless-steel body / any non-corrosive material 2. Should have pump air flow rate minimum 30 – 40/min. 3. Should have vacuum above – 500 mm hg4. Should have three step vacuum adjustments – high, medium and low. 5. Should have secretion container of 2ltr capacity 6. The hose connection between the suction system and secretion jar should be less than 15 cms 7. Should have hygienic bacterial filter with overflow protection 8. Should have sound level maximum of 55 to 65 db 9. Should have motor capacity of minimum of 0.5 HP (1/2 HP) working power of 220/230 V single phase. 10. Should have power supply indicator, suction on indicator, Unit on/off 5amps DP switch, protector fuse and minimum chord length of 5M with 5 Amps 3 pin top. 11. Should be mounted on easy moving castor wheels.	NO	9.00	16240.00	146160.00	17352.00	156168.00	17039.66	153356.98
31	Electrical Cautery Machine:���Monopolar cut: max 400W. Low, Pure, Blend & Endo ii. Monopolar coag: 120W. Desiccate, Fulgurate & Spray iii. Bipolar coag: 120W. Macro, Standard and Precise iv. Bipolar Cut: 100W v. Vessel Seal: L-5, 150W, Auto-stop & regrasp indicators vi. Programmable power settings: 10 programs vii. Tissue sensing technology viii. Patient plate contact quality monitoring ix. HF leakage monitoring Accessories * Silicon Split Patient Plate * Cable for Patient Plate *Disposable handswitch, 3 Pin *Electrode set *Bipolar forcep * Bipolar cable *5mm laparoscopic vessel ealing instrument with cable *Open biclamp with cable *Three-pedal Footswitch	NO	2.00	392000.00	784000.00	418852.00	837704.00	411312.66	822625.33
32	Battery Operated Power Drill (P-Comp with Respac Software)	NO	2.00	168000.00	336000.00	179508.00	359016.00	176276.86	352553.71
33	ENT Microscope (Optive):• Manual 5 Step Magnification changer with apochromatic optics. Magnification Factor 0.4x,0.6x,1.0x,1.6x,2.5x • Objective Lenses f-250mm or 300mm with manual focusing mechanism • Objective Lens Fixed working distance f=400mm • Straight Binacular tube f=170mm interpupillary distance adjustment from 55mm to 75mm • Pair of wide field push –in eyepieces 10x with sleeves and magnetic locks dioptre setting from 6D to -6D • 120 Degree Coupling • Front Hand Grip • Coaxial Fiber Optic Illumination System with LED Illumination. • Stable and study floor stand on four lockable castors, column Spring Balance articulated arm, Carrier arm Power supply , unit Light Guide ,2m power cable .	NO	1.00	728000.00	728000.00	777868.00	777868.00	763866.38	763866.38

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rate Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
34	Otoscope Welch Allyn:◆◆◆◆◆◆◆◆◆◆ 1.◆◆◆◆◆◆◆◆◆ Should be a convenient pocket type otoscope.◆◆◆◆◆◆◆◆◆◆ 2.◆◆◆◆◆◆◆◆◆ Should be provided with a halogen light source.◆◆◆◆◆◆◆◆◆◆ 3.◆◆◆◆◆◆◆◆◆ Should be able to detach the otoscope head.◆◆◆◆◆◆◆◆◆◆ 4.◆◆◆◆◆◆◆◆◆ Should provide no reflections and obstructions.◆◆◆◆◆◆◆◆◆◆ 5.◆◆◆◆◆◆◆◆◆ Should provide detachable accessories of various sizes.◆◆◆◆◆◆◆◆◆◆ 6.◆◆◆◆◆◆◆◆◆ Should have in built rechargeable battery. Recharge should be possible with direct mains supply	NO	1.00	264320.00	264320.00	282426.00	282426.00	277342.33	277342.33
35	Oxygen Flow meter with Regulator:◆◆ 1.◆◆◆◆◆◆◆◆◆ Internal reseating relief valve protects against over-pressurization◆◆◆◆◆◆◆◆◆◆ 2.◆◆◆◆◆◆◆◆◆ Sintered filter for additional safety and to extend regulator life◆◆◆◆◆◆◆◆◆ 3.◆◆◆◆◆◆◆◆◆ 2in Diameter gauge◆◆◆◆◆◆◆◆◆◆ 4.◆◆◆◆◆◆◆◆◆ 15LPM Oxygen models provide 85 to 90LPM flood maximum◆◆◆◆◆◆◆◆◆◆ 5.◆◆◆◆◆◆◆◆◆ 7LPM models restricted to 10LPM maximum	NO	12.00	2800.00	33600.00	2992.00	35904.00	2938.14	35257.73
36	ECG MACHINE :◆◆◆ 1.◆◆◆◆◆◆◆◆◆ Simultaneous 12 Channel ECG recording with 12 lead simultaneous acquisition◆◆◆◆◆◆◆◆◆◆ 2.◆◆◆◆◆◆◆◆◆ Should have visual alarm for open lead◆◆◆◆◆◆◆◆◆◆ 3.◆◆◆◆◆◆◆◆◆ Should have a digital display of 12 channel ECG◆◆◆◆◆◆◆◆◆◆ 4.◆◆◆◆◆◆◆◆◆ QWERTY Alphanumeric keyboard◆◆◆◆◆◆◆◆◆◆ 5.◆◆◆◆◆◆◆◆◆ Built-in ECG Parameters measurements and Interpretation◆◆◆◆◆◆◆◆◆◆ 6.◆◆◆◆◆◆◆◆◆ Minimum 40 ECG Storage inbuilt memory.◆◆◆◆◆◆◆◆◆◆ 7.◆◆◆◆◆◆◆◆◆ 3 Operating modes: Automatic, Manual and Rhythm◆◆◆◆◆◆◆◆◆◆ 8.◆◆◆◆◆◆◆◆◆ Should have a maintenance free digital thermal array printer◆◆◆◆◆◆◆◆◆◆ 9.◆◆◆◆◆◆◆◆◆ Printer should work with standard thermal paper (should be available in Local Market)◆◆◆◆◆◆◆◆ 10.◆◆◆◆◆◆◆◆ Should have 12 lead ECG preview display before taking printouts and should have printer on/off selection.◆◆◆◆◆◆◆◆ 11.◆◆◆◆◆◆◆◆ Should have ECG lead annotation facility◆◆◆◆◆◆◆◆ 12.◆◆◆◆◆◆◆◆ Machine should have sufficient battery backup for taking at least 25 nos ECG on a fully charged battery ◆◆◆◆◆◆◆◆ 13.◆◆◆◆◆◆◆◆ Should supplied with 2 patient cable sets, 8 clips on electrodes, 12 chest electrodes with silicone rubber bulb, 12 packets of recording paper,1 bottle of jelly and 12 nos. reusable button type electrode◆◆◆◆◆◆◆◆ 14.◆◆◆◆◆◆◆◆ Should operate on mains(220v-50Hz) and rechargeable battery	NO	6.00	134400.00	806400.00	152000.00	912000.00	149264.00	895584.00

Scanned by TapScanner

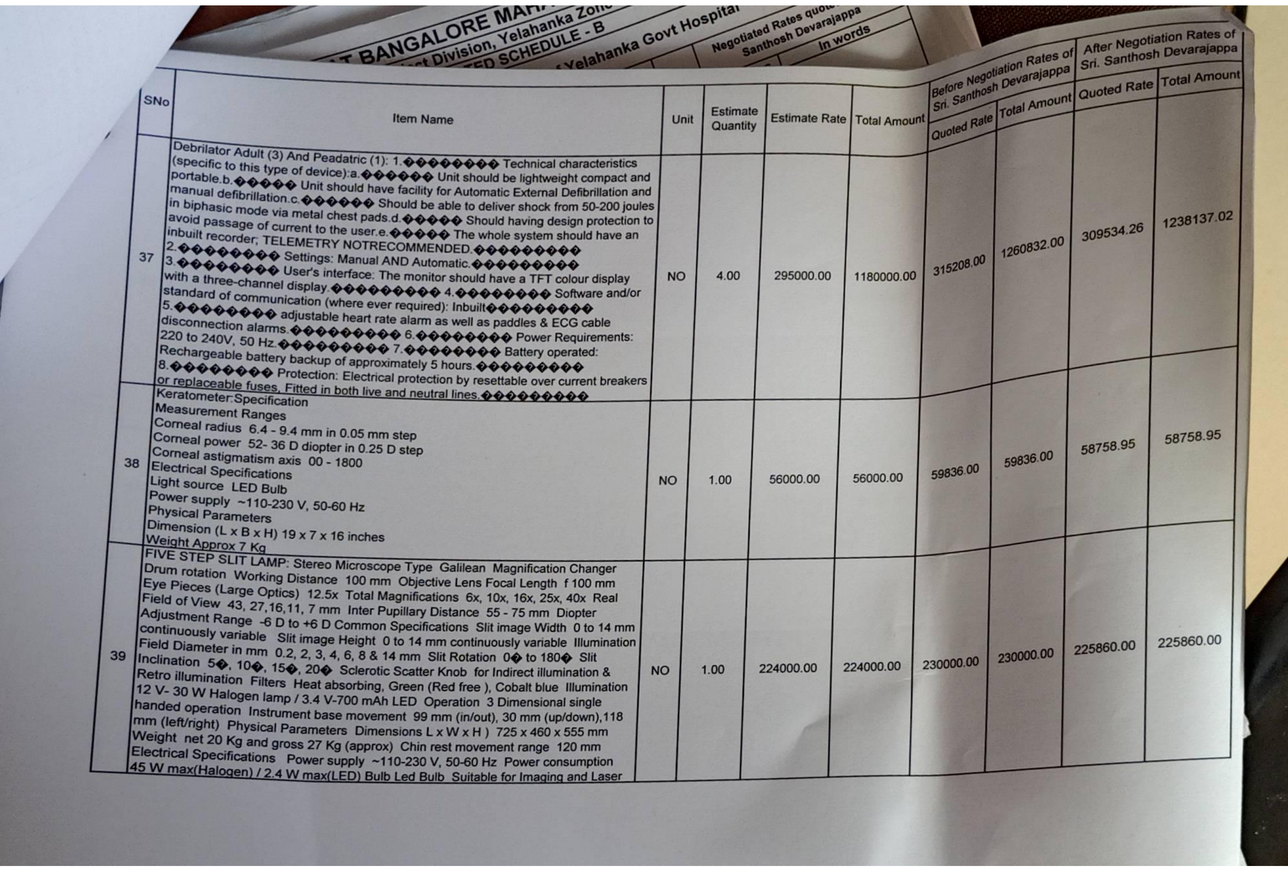

BANGALORE MAH...
...t Division, Yelahanka Zon...
...ED SCHEDULE - B
...Yelahanka Govt Hospital
Negotiated Rates quot...
Santhosh Devarajappa
In words

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
37	Debrilator Adult (3) And Peadatric (1): 1.◆◆◆◆◆◆◆◆◆ Technical characteristics (specific to this type of device):a.◆◆◆◆◆◆◆ Unit should be lightweight compact and portable.b.◆◆◆◆◆ Unit should have facility for Automatic External Defibrillation and manual defibrillation.c.◆◆◆◆◆◆◆ Should be able to deliver shock from 50-200 joules in biphasic mode via metal chest pads.d.◆◆◆◆◆ Should having design protection to avoid passage of current to the user.e.◆◆◆◆◆ The whole system should have an inbuilt recorder; TELEMETRY NOTRECOMMENDED.◆◆◆◆◆◆◆◆◆ 2.◆◆◆◆◆◆◆◆◆ Settings: Manual AND Automatic.◆◆◆◆◆◆◆◆◆ 3.◆◆◆◆◆◆◆◆◆ User's interface: The monitor should have a TFT colour display with a three-channel display.◆◆◆◆◆◆◆◆◆ 4.◆◆◆◆◆◆◆◆◆ Software and/or standard of communication (where ever required): Inbuilt◆◆◆◆◆◆◆◆◆ 5.◆◆◆◆◆◆◆◆◆ adjustable heart rate alarm as well as paddles & ECG cable disconnection alarms.◆◆◆◆◆◆◆◆◆ 6.◆◆◆◆◆◆◆◆◆ Power Requirements: 220 to 240V, 50 Hz.◆◆◆◆◆◆◆◆◆ 7.◆◆◆◆◆◆◆◆◆ Battery operated: Rechargeable battery backup of approximately 5 hours.◆◆◆◆◆◆◆◆◆ 8.◆◆◆◆◆◆◆◆◆ Protection: Electrical protection by resettable over current breakers or replaceable fuses. Fitted in both live and neutral lines.◆◆◆◆◆◆◆◆◆	NO	4.00	295000.00	1180000.00	315208.00	1260832.00	309534.26	1238137.02
38	Keratometer:Specification Measurement Ranges Corneal radius 6.4 - 9.4 mm in 0.05 mm step Corneal power 52- 36 D diopter in 0.25 D step Corneal astigmatism axis 00 - 1800 Electrical Specifications Light source LED Bulb Power supply ~110-230 V, 50-60 Hz Physical Parameters Dimension (L x B x H) 19 x 7 x 16 inches Weight Approx 7 Kg	NO	1.00	56000.00	56000.00	59836.00	59836.00	58758.95	58758.95
39	FIVE STEP SLIT LAMP: Stereo Microscope Type Galilean Magnification Changer Drum rotation Working Distance 100 mm Objective Lens Focal Length f 100 mm Eye Pieces (Large Optics) 12.5x Total Magnifications 6x, 10x, 16x, 25x, 40x Real Field of View 43, 27,16,11, 7 mm Inter Pupillary Distance 55 - 75 mm Diopter Adjustment Range -6 D to +6 D Common Specifications Slit image Width 0 to 14 mm continuously variable Slit image Height 0 to 14 mm continuously variable Illumination Field Diameter in mm 0.2, 2, 3, 4, 6, 8 & 14 mm Slit Rotation 0◆ to 180◆ Slit Inclination 5◆, 10◆, 15◆, 20◆ Sclerotic Scatter Knob for Indirect illumination & Retro illumination Filters Heat absorbing, Green (Red free), Cobalt blue Illumination 12 V- 30 W Halogen lamp / 3.4 V-700 mAh LED Operation 3 Dimensional single handed operation Instrument base movement 99 mm (in/out), 30 mm (up/down),118 mm (left/right) Physical Parameters Dimensions L x W x H) 725 x 460 x 555 mm Weight net 20 Kg and gross 27 Kg (approx) Chin rest movement range 120 mm Electrical Specifications Power supply ~110-230 V, 50-60 Hz Power consumption 45 W max(Halogen) / 2.4 W max(LED) Bulb Led Bulb Suitable for Imaging and Laser	NO	1.00	224000.00	224000.00	230000.00	230000.00	225860.00	225860.00

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
40	FLASH AUTO CLAVE:Size -Overall W = 40 to 50cm L = 40 to 50cm H = 30 to 40cm approx -Chamber 20cm x 35cm L approx. Electrical: -Supply 220-240V Construction Stainless steel chamber, door and trays Instrumentation Cycle status display. Digital temperature display, Pressure guage, Safety Pressure safety valve, Door safety catch, Overheat Protection with warning indicator, Chamber pressure indicator, Pressure door lock. Sterilizing: -Sterilizing time: At 134 deg.C———5 to 12 min; At 121 deg.C———15 to 25 min. Drying time approx 15minutes when selected	NO	1.00	413000.00	413000.00	441291.00	441291.00	433347.76	433347.76
41	TENS (BOTH FARADIC & GALVANIC):Advanced Programmed T..E.. N.. S.. Therapy Unit (Dual Channel)LCD Display12 preset PrograMeBurst100HZBurst 200 HzConstant 2HzConstant 10 HzConstant 20 HzConstant 40 HzConstant 80 HZConstant 100 HzConstant 120 HzConstant 150 HzSurge 100HzSurge 200 HzPower supply : 90V to 270V (SMPS Power supply)Unit will be supplied with all standard accessories :Main Unit : 01 No.Electrodes : 04 Nos.Main cable : 01 No.Wire Set : 02 Nos. (4 output)Power Socketwill be provided free of cost as per country requirement.	NO	1.00	23180.64	23180.64	24000.00	24000.00	23568.00	23568.00
42	NST Machine with probe :�� 1.��������� It should have Numerical display of FHR, TOCO & Foetal Movements Counts��������� 2.��������� It should have min of 15cm Display for displaying Wave forms of FHR & TOCO��������� 3.��������� It should have Automatic Foetal Movement Detection��������� 4.��������� It should have minimum of 2 Hours Battery Backup��������� 5.��������� It should be provided with Computer Foetal monitoring Software and Data cable for storage & Reload��������� 6.��������� It should be easy to use & take print out��������� 7.��������� It should have inbuilt Thermal recorder��������� 8.��������� It should have inbuilt memory of 10 Hrs Graphical Recording��������� 9.��������� It should be provided with Aluminium cart with wheels for easy Movement of the machine������ 10.��������� It should have built in Network Capability������ 11.��������� Should be BIS / CE / FDA certified product.	NO	2.00	129800.00	259600.00	130000.00	260000.00	127660.00	255320.00

Scanned by TapScanner

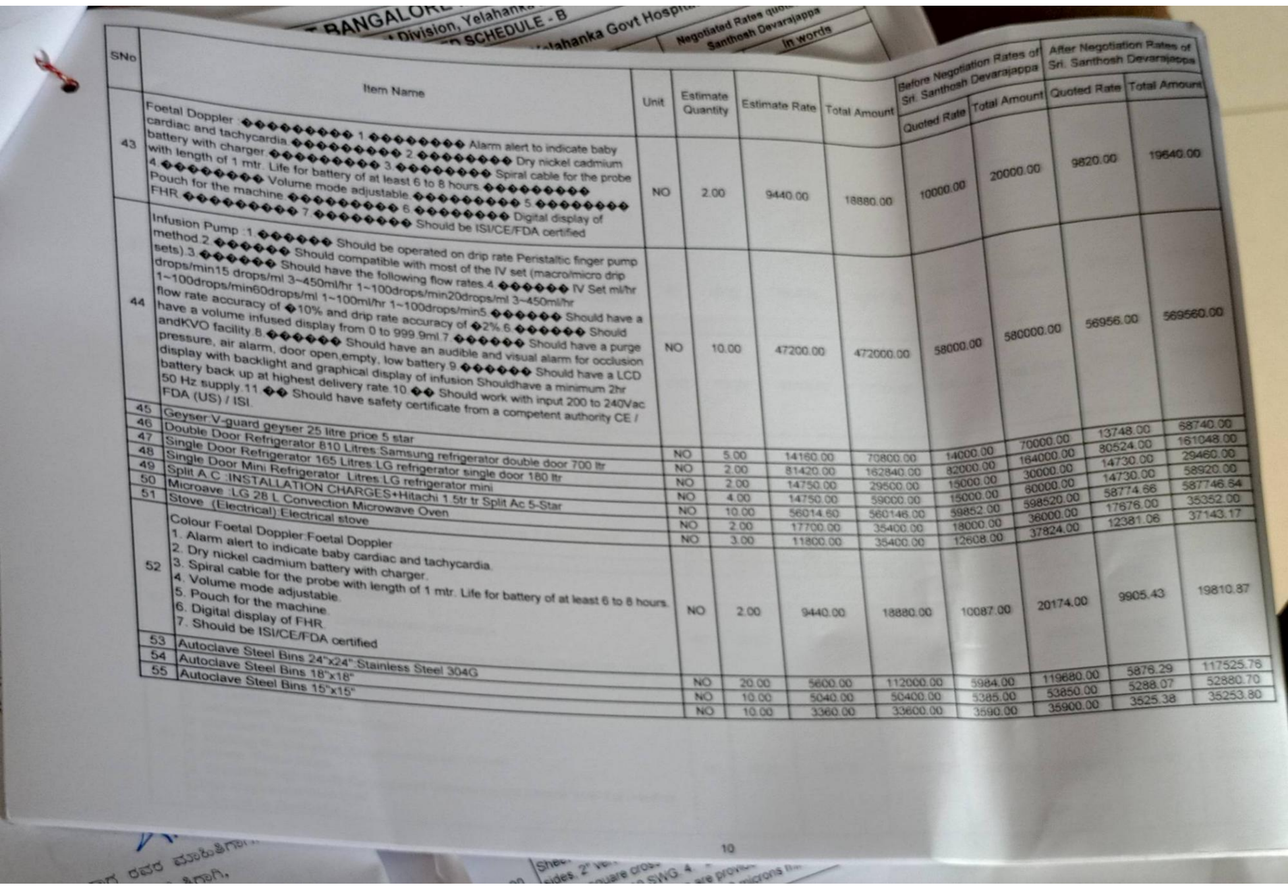

RANGALORE
Division, Yelahanka
SCHEDULE - 8
Yelahanka Govt Hospital
Negotiated Rates quoted by Sri. Santhosh Devarajappa
in words

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
43	Foetal Doppler :1.◆◆◆◆◆◆◆◆◆◆ 1.◆◆◆◆◆◆◆◆◆ Alarm alert to indicate baby cardiac and tachycardia.◆◆◆◆◆◆◆◆◆◆ 2.◆◆◆◆◆◆◆◆◆ Dry nickel cadmium battery with charger.◆◆◆◆◆◆◆◆◆◆ 3.◆◆◆◆◆◆◆◆◆ Spiral cable for the probe with length of 1 mtr. Life for battery of at least 6 to 8 hours.◆◆◆◆◆◆◆◆◆◆ 4.◆◆◆◆◆◆◆◆◆ Volume mode adjustable.◆◆◆◆◆◆◆◆◆◆ 5.◆◆◆◆◆◆◆◆◆ Pouch for the machine.◆◆◆◆◆◆◆◆◆◆ 6.◆◆◆◆◆◆◆◆◆◆ 7.◆◆◆◆◆◆◆◆◆ Digital display of FHR.◆◆◆◆◆◆◆◆◆◆ 8.◆◆◆◆◆◆◆◆◆◆ 9.◆◆◆◆◆◆◆◆◆ Should be ISI/CE/FDA certified	NO	2.00	9440.00	18880.00	10000.00	20000.00	9820.00	19640.00
44	Infusion Pump :1.◆◆◆◆◆◆◆ Should be operated on drip rate Peristaltic finger pump method.2.◆◆◆◆◆◆◆ Should compatible with most of the IV set (macro/micro drip sets).3.◆◆◆◆◆◆◆ Should have the following flow rates.4.◆◆◆◆◆◆◆ IV Set ml/hr drops/min15 drops/ml 3~450ml/hr 1~100drops/min20drops/ml 3~450ml/hr 1~100drops/min60drops/ml 1~100ml/hr 1~100drops/min5.◆◆◆◆◆◆◆ Should have a flow rate accuracy of ◆10% and drip rate accuracy of ◆2%.6.◆◆◆◆◆◆◆ Should have a volume infused display from 0 to 999.9ml.7.◆◆◆◆◆◆◆ Should have a purge andKVO facility.8.◆◆◆◆◆◆◆ Should have an audible and visual alarm for occlusion pressure, air alarm, door open,empty, low battery.9.◆◆◆◆◆◆◆ Should have a LCD display with backlight and graphical display of infusion Shouldhave a minimum 2hr battery back up at highest delivery rate.10.◆◆ Should work with input 200 to 240Vac 50 Hz supply.11.◆◆ Should have safety certificate from a competent authority CE / FDA (US) / ISI.	NO	10.00	47200.00	472000.00	58000.00	580000.00	56956.00	569560.00
45	Geyser:V-guard geyser 25 litre price 5 star	NO	5.00	14160.00	70800.00	14000.00	70000.00	13748.00	68740.00
46	Double Door Refrigerator 810 Litres:Samsung refrigerator double door 700 ltr	NO	2.00	81420.00	162840.00	82000.00	164000.00	80524.00	161048.00
47	Single Door Refrigerator 165 Litres:LG refrigerator single door 180 ltr	NO	2.00	14750.00	29500.00	15000.00	30000.00	14730.00	29460.00
48	Single Door Mini Refrigerator_Litres:LG refrigerator mini	NO	4.00	14750.00	59000.00	15000.00	60000.00	14730.00	58920.00
49	Split A.C._INSTALLATION CHARGES+Hitachi 1.5tr tr Split Ac 5-Star	NO	10.00	56014.60	560146.00	59852.00	598520.00	58774.66	587746.64
50	Microave :LG 28 L Convection Microwave Oven	NO	2.00	17700.00	35400.00	18000.00	36000.00	17676.00	35352.00
51	Stove (Electrical):Electrical stove	NO	3.00	11800.00	35400.00	12608.00	37824.00	12381.06	37143.17
52	Colour Foetal Doppler:Foetal Doppler 1. Alarm alert to indicate baby cardiac and tachycardia. 2. Dry nickel cadmium battery with charger. 3. Spiral cable for the probe with length of 1 mtr. Life for battery of at least 6 to 8 hours. 4. Volume mode adjustable. 5. Pouch for the machine. 6. Digital display of FHR. 7. Should be ISI/CE/FDA certified	NO	2.00	9440.00	18880.00	10087.00	20174.00	9905.43	19810.87
53	Autoclave Steel Bins 24"x24" Stainless Steel 304G	NO	20.00	5600.00	112000.00	5984.00	119680.00	5876.29	117525.76
54	Autoclave Steel Bins 18"x18"	NO	10.00	5040.00	50400.00	5385.00	53850.00	5288.07	52880.70
55	Autoclave Steel Bins 15"x15"	NO	10.00	3360.00	33600.00	3590.00	35900.00	3525.38	35253.80

10

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
56	Bedside Lockers:Bed Side Locker 1. Size: H32" x W16" x D16" 2. Size of the Cupboard: H16" x W14"x D16" located in the centre 3. Cupboard made of CRCA steel sheet with double hinged door and locker facility 4. Locker top to have S.S. Sheet super imposed with raised edges on three sides 5. Framework of 1" square M.S. and legs with rubber feet. Full frame and cupboard to be powder coated in Seamen's Grey colour with 50 microns coating. 6. Should be ISI / CE Certified	NO	60.00	2360.00	141600.00	2522.00	151320.00	2476.60	148596.24
57	Stainless Steel Foot Step:Stainless Steel Foot Step 1. Overall size: 18"X9"X20" 2. TOP SHEET: 18 gauge S.S. 3. DESIGN: Top fitted with aluminium tread flats. Height 9" and 20" 1" Sq.16 SWG SS Pipes to be used. 4 Nos. Nylon feet 4. Should be ISI / CE Certified	NO	10.00	1502.70	15027.00	1606.00	16060.00	1577.09	15770.92
58	Powder Coated Back Rest:Size 78Lx36Wx24H, Back Rest by Screw rod Mechanism, Powder coated Uniformly perforated Two Sectional CRCA sheet top, Frame work made of Rectangular M.S. Tube, ABS Bow, Collaociable side Railings The above product should conform to applicable ISI Standards in respect of materials, welding process, tests and performance, Finish: Pretreated and Epoxy Powder Coated to be supplied along with Matterss 3' coir n 1" foam	NO	10.00	17700.00	177000.00	18912.00	189120.00	18571.58	185715.84
59	Foot End Elevators:Size 78Lx36Wx24H, Back Rest & Knee rest by Screw rod Mechanism, Powder coated Uniformly perforated four sectional CRCA sheet top, Frame work made of Rectangular M.S. Tube, ABS Bow, Collaociable side Railings The above product should conform to applicable ISI Standards in respect of materials, welding process, tests and performance, Finish: Pretreated and Epoxy Powder Coated to be supplied along with Matterss 3' coir n 1" foam	NO	10.00	41300.00	413000.00	48500.00	485000.00	47627.00	476270.00
60	Plastic Bed Pans	NO	20.00	280.00	5600.00	300.00	6000.00	294.60	5892.00
61	Plastic Urine Can	NO	20.00	112.00	2240.00	120.00	2400.00	117.84	2356.80
62	Needle Holder 8" :Length: 8" b. Tip Configuration: Blunt c. Instruments Type: Needle Holder d. Curvature: Straight e. Working Surface Style: Cross-Serrated with Groove f. Handle: Finger Rings g. Should be high Quality Surgical steel Instruments and Manufactured from medical grade surgical stainless steel h. Should be Sterilizable	NO	20.00	560.00	11200.00	600.00	12000.00	589.20	11784.00
63	Needle Holder 6" ,:Length: 6" b. Tip Configuration: Blunt c. Instruments Type: Needle Holder d. Curvature: Straight e. Working Surface Style: Cross-Serrated with Groove f. Handle: Finger Rings g. Should be high Quality Surgical steel Instruments and Manufactured from medical grade surgical stainless steel h. Should be Sterilizable	NO	50.00	448.00	22400.00	500.00	25000.00	491.00	24550.0

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
64	Allis Forceps 4":Length: 4" b. Instrument Type: Allis Forceps 4" c. Curvature: Straight d. Handle: Finger Rings e. Should be High Quality Surgical Steel Instruments and Manufactured from medical grade Surgical Stainless steel f. Should be Sterilizable	NO	250.00	392.00	98000.00	400.00	100000.00	392.80	98200.00
65	Cockers St 7":Length: 7" b. Instrument Type: Cockers St 7" c. Curvature: Straight d. Handle: Finger Rings e. Should be High Quality Surgical Steel Instruments and Manufactured from medical grade Surgical Stainless steel f. Should be Sterilizable	NO	50.00	672.00	33600.00	700.00	35000.00	687.40	34370.00
66	Cockers CURVED 7":Length: 7" b. Instrument Type: Cockers St 7" c. Curvature: Curved d. Handle: Finger Rings e. Should be High Quality Surgical Steel Instruments and Manufactured from medical grade Surgical Stainless steel f. Should be Sterilizable	NO	50.00	672.00	33600.00	700.00	35000.00	687.40	34370.00
67	Scissors Fine Tip 7":Size: 7" b. Curvature: fine tip c. Fully graduated in centimetres d. Should be high Quality Surgical steel instrument and Manufactured from medical grade surgical stainless steel e. Should be Sterilizable	NO	20.00	728.00	14560.00	750.00	15000.00	736.50	14730.00
68	Scissors Straight 7":Size: 7" b. Curvature: Straight c. Fully graduated in centimetres d. Should be high Quality Surgical steel instrument and Manufactured from medical grade surgical stainless steel e. Should be Sterilizable	NO	30.00	728.00	21840.00	750.00	22500.00	736.50	22095.00
69	Scissors 6" curved:Size: 6" b. Curvature: Curved c. Fully graduated in centimetres d. Should be high Quality Surgical steel instrument and Manufactured from medical grade surgical stainless steel e. Should be Sterilizable	NO	25.00	672.00	16800.00	700.00	17500.00	687.40	17185.00
70	Scissors Fine Tip 5":Size: 5" b. Curvature: fine tip c. Fully graduated in centimetres d. Should be high Quality Surgical steel instrument and Manufactured from medical grade surgical stainless steel e. Should be Sterilizable	NO	20.00	672.00	13440.00	700.00	14000.00	687.40	13748.00

Scanned by TapScanner

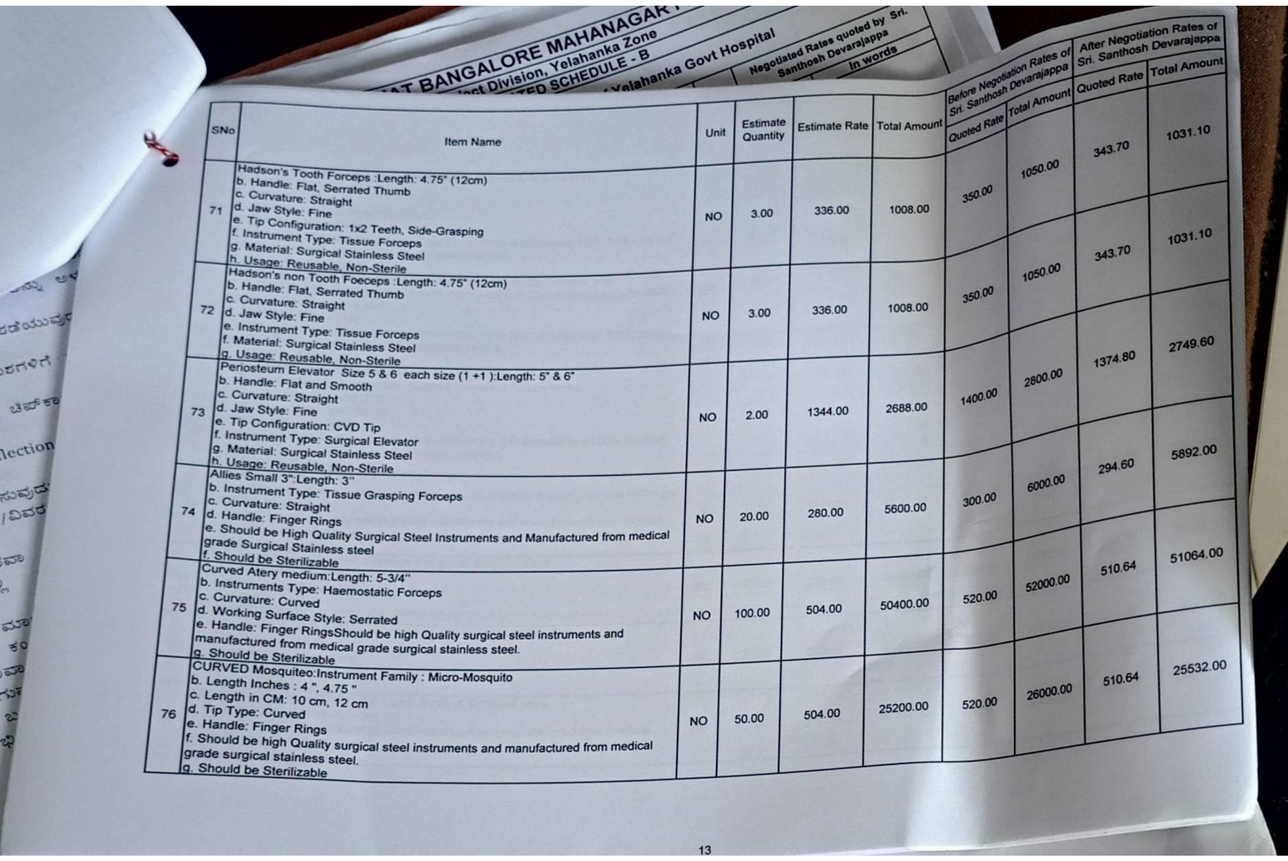

...AT BANGALORE MAHANAGAR ...
...ject Division, Yelahanka Zone
...TED SCHEDULE - B
...Yelahanka Govt Hospital

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Negotiated Rates quoted by Sri. Santhosh Devarajappa in words		Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
								Quoted Rate	Total Amount	Quoted Rate	Total Amount
71	Hadson's Tooth Forceps :Length: 4.75" (12cm) b. Handle: Flat, Serrated Thumb c. Curvature: Straight d. Jaw Style: Fine e. Tip Configuration: 1x2 Teeth, Side-Grasping f. Instrument Type: Tissue Forceps g. Material: Surgical Stainless Steel h. Usage: Reusable, Non-Sterile	NO	3.00	336.00	1008.00			350.00	1050.00	343.70	1031.10
72	Hadson's non Tooth Foeceps :Length: 4.75" (12cm) b. Handle: Flat, Serrated Thumb c. Curvature: Straight d. Jaw Style: Fine e. Instrument Type: Tissue Forceps f. Material: Surgical Stainless Steel g. Usage: Reusable, Non-Sterile	NO	3.00	336.00	1008.00			350.00	1050.00	343.70	1031.10
73	Periosteum Elevator Size 5 & 6 each size (1 +1):Length: 5" & 6" b. Handle: Flat and Smooth c. Curvature: Straight d. Jaw Style: Fine e. Tip Configuration: CVD Tip f. Instrument Type: Surgical Elevator g. Material: Surgical Stainless Steel h. Usage: Reusable, Non-Sterile	NO	2.00	1344.00	2688.00			1400.00	2800.00	1374.80	2749.60
74	Allies Small 3":Length: 3" b. Instrument Type: Tissue Grasping Forceps c. Curvature: Straight d. Handle: Finger Rings e. Should be High Quality Surgical Steel Instruments and Manufactured from medical grade Surgical Stainless steel f. Should be Sterilizable	NO	20.00	280.00	5600.00			300.00	6000.00	294.60	5892.00
75	Curved Atery medium:Length: 5-3/4" b. Instruments Type: Haemostatic Forceps c. Curvature: Curved d. Working Surface Style: Serrated e. Handle: Finger RingsShould be high Quality surgical steel instruments and manufactured from medical grade surgical stainless steel. g. Should be Sterilizable	NO	100.00	504.00	50400.00			520.00	52000.00	510.64	51064.00
76	CURVED Mosquiteo:Instrument Family : Micro-Mosquito b. Length Inches : 4 ", 4.75 " c. Length in CM: 10 cm, 12 cm d. Tip Type: Curved e. Handle: Finger Rings f. Should be high Quality surgical steel instruments and manufactured from medical grade surgical stainless steel. g. Should be Sterilizable	NO	50.00	504.00	25200.00			520.00	26000.00	510.64	25532.00

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		Sri. Sant	
						Quoted Rate	Total Amount	Quoted Rate	Total Amt
77	Copper Handed Curved ARTERY Medium :Curved Artery medium b. Length: 5-3/4" c. Curvature: Curved d. Working Surface Style: Serrated e. Handle: Finger Rings f. Should be high Quality surgical steel instruments and manufactured from medical grade surgical stainless steel with tungsten carbide. g. Should be Sterilizable	NO	15.00	616.00	9240.00	620.00	9300.00	608.84	9132.6
78	Langen Back Right Angle Retractor different Sizes:Length: different size b. Should be high Quality surgical steel instrument and Manufactured from medical grade surgical stainless steel c. should be Sterilizable d. Should be high Quality surgical steel instruments and manufactured from medical grade surgical stainless steel with tungsten carbide. e. Should be Sterilizable	NO	30.00	840.00	25200.00	860.00	25800.00	844.52	25335
79	Mayo's Retractor:Composition: Stainless b. Customer Segment: Hospitals, Surgery Centers & Tissue Banks c. Length - Overall (mm): 275 d. Physician/Developer: Mayo e. Shape: Right-Angled f. Should be high Quality surgical steel instruments and manufactured from medical grade surgical stainless steel with tungsten carbide. g. Should be Sterilizable	NO	5.00	1344.00	6720.00	1360.00	6800.00	1335.52	6677
80	Dever's Retractor:Size: 12X1 b. Used to retract liver in surgical procedures like cholecystectomy (removal of the gall bladder), vagotomy c. Should be high Quality surgical steel instruments and manufactured from medical grade surgical stainless steel. d. Should be Sterilizable	NO	5.00	1344.00	6720.00	1360.00	6800.00	1335.52	6677
81	Disecting Forceps Toothed :Made of 410 grade stainless steel. b. Total length – 15 cm c. Sand blasting from inside d. Tip should be 2x1 e. Matt/ dull finish	NO	100.00	280.00	28000.00	290.00	29000.00	284.78	2847
82	Disecting Forceps non Toothed :Made of 410 grade stainless steel. b. Total length – 15 cm c. Sand blasting from inside d. Tip should be 2x1 e. Matt/ dull finish	NO	100.00	280.00	28000.00	290.00	29000.00	284.78	284
83	Sponge Holder :Size: 9-1/2" (24.1 cm), Straight, Serrated Jaws b. Fully graduated in centimetres c. Should be high quality surgical steel Instrument and manufactured from medical grade Surgical stainless steel d. Should be Sterilizable	NO	70.00	840.00	58800.00	850.00	59500.00	834.70	584

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
84	Speculum Medium :Shape: Should be Double Ended b. Size: Should be medium in size (blade one size 75x30mm, other 80x35 mm) c. Material: Should be high Quality Surgical steel instrument and manufactured from medical grade surgical Stainless steel d. Safety: Protects Patients against Cross infection risks. e. Use: Should be reusable	NO	60.00	1344.00	80640.00	1360.00	81600.00	1335.52	80131.20
85	Anterior Vaginal wall Retractor:Made of 410 Grade Stainless Steel b. Total Length – 25.5CM c. Rings should be oval shaped d. Both sides serrated rings e. Ring internal diameter – 15MM & 18MM f. Matt/ Dull Finish	NO	13.00	1120.00	14560.00	1140.00	14820.00	1119.48	14553.24
86	Tubual Ligation Set	NO	1.00	8400.00	8400.00	8500.00	8500.00	8347.00	8347.00
87	Surgical D &C Set	NO	1.00	9520.00	9520.00	10000.00	10000.00	9820.00	9820.00
88	B.P.Handle big:Forgings from Stainless Steel. b. Silk Matte Satin Finish. c. To Hold Scalpel Blades. d. Used Mostly In All Surgery.	NO	30.00	280.00	8400.00	300.00	9000.00	294.60	8838.00
89	B.P. Handle small:Forgings from Stainless Steel. b. Silk Matte Satin Finish. c. To Hold Scalpel Blades. d. Used Mostly In All Surgery.	NO	10.00	224.00	2240.00	240.00	2400.00	235.68	2356.80
90	Varicose Veins Stripper	NO	2.00	11200.00	22400.00	11500.00	23000.00	11293.00	22586.00
91	Ovum Foeceps (gynec):Size: 9-1/2" (24.1 cm), Straight, Serrated Jaws b. Fully graduated in centimetres c. Should be high quality surgical steel Instrument and manufactured from medical grade Surgical stainless steel d. Should be Sterilizable	NO	2.00	1344.00	2688.00	1360.00	2720.00	1335.52	2671.04
92	Cord Cutting Scissors:Should be very wide blades with large, rounded, blunt tips that slide past each other b. The blades are attached to handles with the proximal end conformed as a ring to facilitate holding and operating with the fingers; both parts are joined by a swivel pin in the centre. c. Should be high quality surgical steel Instrument and manufactured from medical grade Surgical stainless steel d. Should be Sterilizable	NO	20.00	616.00	12320.00	620.00	12400.00	608.84	12176.80
93	Episcotmy Scissiors:Made of 420 grade stainless steel b. ISI/CE/FDA certified & anti rust instrument c. Total length – 14 cm d. Blade length – 4.6 cm e. Blades should be angled f. Rings should be smooth g. Matt/ dull finish	NO	25.00	672.00	16800.00	690.00	17250.00	677.58	16939.50
94	Cervical Biopsy Set	NO	2.00	2800.00	5600.00	2900.00	5800.00	2847.80	5695.60
95	Steel Trays medium :Instrument Tray with cover – Stainless steel of 304 grade b. Size: 300x 200 x 65mm	NO	60.00	560.00	33600.00	580.00	34800.00	569.56	34173.60

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates Sri. Santhosh Devarajappa		Sri. Sa...	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
96	Cheatle Forceps Made of 410 grade stainless steel b. ISI/CE/FDA certified & anti rust instrument c. Total length – 25.5 cm d. Jaw length – 7.8 cm e. Jaws should be smooth without serration f. Rings should be smooth g. Matt/ dull finish	NO	20.00	840.00	16800.00	860.00	17200.00	844.52	16890.40
97	Suction Tips Different Size:Tubing Material: Medical-grade Polyvinyl Chloride (PVC) Plastic b. tubing size 1/4", length 1.80m, Yankauer handle with control vent and crown tip c. tubing size 1/4", length 3.60m, Yankauer handle with control vent and crown tip d. tubing size 3/16", length 1.80m, Yankauer handle with control vent and crown tip e. tubing size 3/16", length 3.60m, Yankauer handle with control vent and crown tip	NO	10.00	560.00	5600.00	580.00	5800.00	569.56	5695.60
98	Laryango Scope with Blades ADULT:Handle: stainless steel or chromium-plated, slightly rigged. b. Depressor and laryngoscope blade: stainless steel, curved or straight. c. Complete, ready-to-use, the laryngoscope should be L-shaped so that the handle and batteries are at a right angle to the blade. d. Illumination: battery compartment in the handle, lamp positioned on the blade. e. An instrument used to inspect the larynx, comprised of a: - Hollow handle, 2-battery compartment type. - Spatula or blade: f. Macintosh type: slightly curved blade with a small bulbous tip, fixed to a hook-on handle. g. Each blade has a single bulb, removable for cleaning.	NO	21.00	2800.00	58800.00	2900.00	60900.00	2847.80	59803.80
99	Laryango Scope with Blades Peadeatric:Handle: stainless steel or chromium-plated, slightly rigged. b. Depressor and laryngoscope blade: stainless steel, curved or straight. c. Complete, ready-to-use, the laryngoscope should be L-shaped so that the handle and batteries are at a right angle to the blade. d. Illumination: battery compartment in the handle, lamp positioned on the blade. e. An instrument used to inspect the larynx, comprised of a: - Hollow handle, 2-battery compartment type. - Spatula or blade: f. Macintosh type: slightly curved blade with a small bulbous tip, fixed to a hook-on handle. g. Each blade has a single bulb, removable for cleaning.	NO	11.00	2800.00	30800.00	2900.00	31900.00	2847.80	31325.80
100	Ambu bag Adult /Peadtric Set (10 +10):700ml and 200ml Self inflating double ended silicone bag with mounts b. Side feed oxygen inlet c. Type "L" non-rebreathing valve with pressure limiting device 40cms of water d. Size 0A Circular Pedi All Silicone facemask e. Reservoir Hose with Adaptor to provide higher oxygen & 1.5mtrs oxygen enrichment tubing f. Carrying case	NO	20.00	1400.00	28000.00	1450.00	29000.00	1423.90	28478.00

Scanned by TapScanner

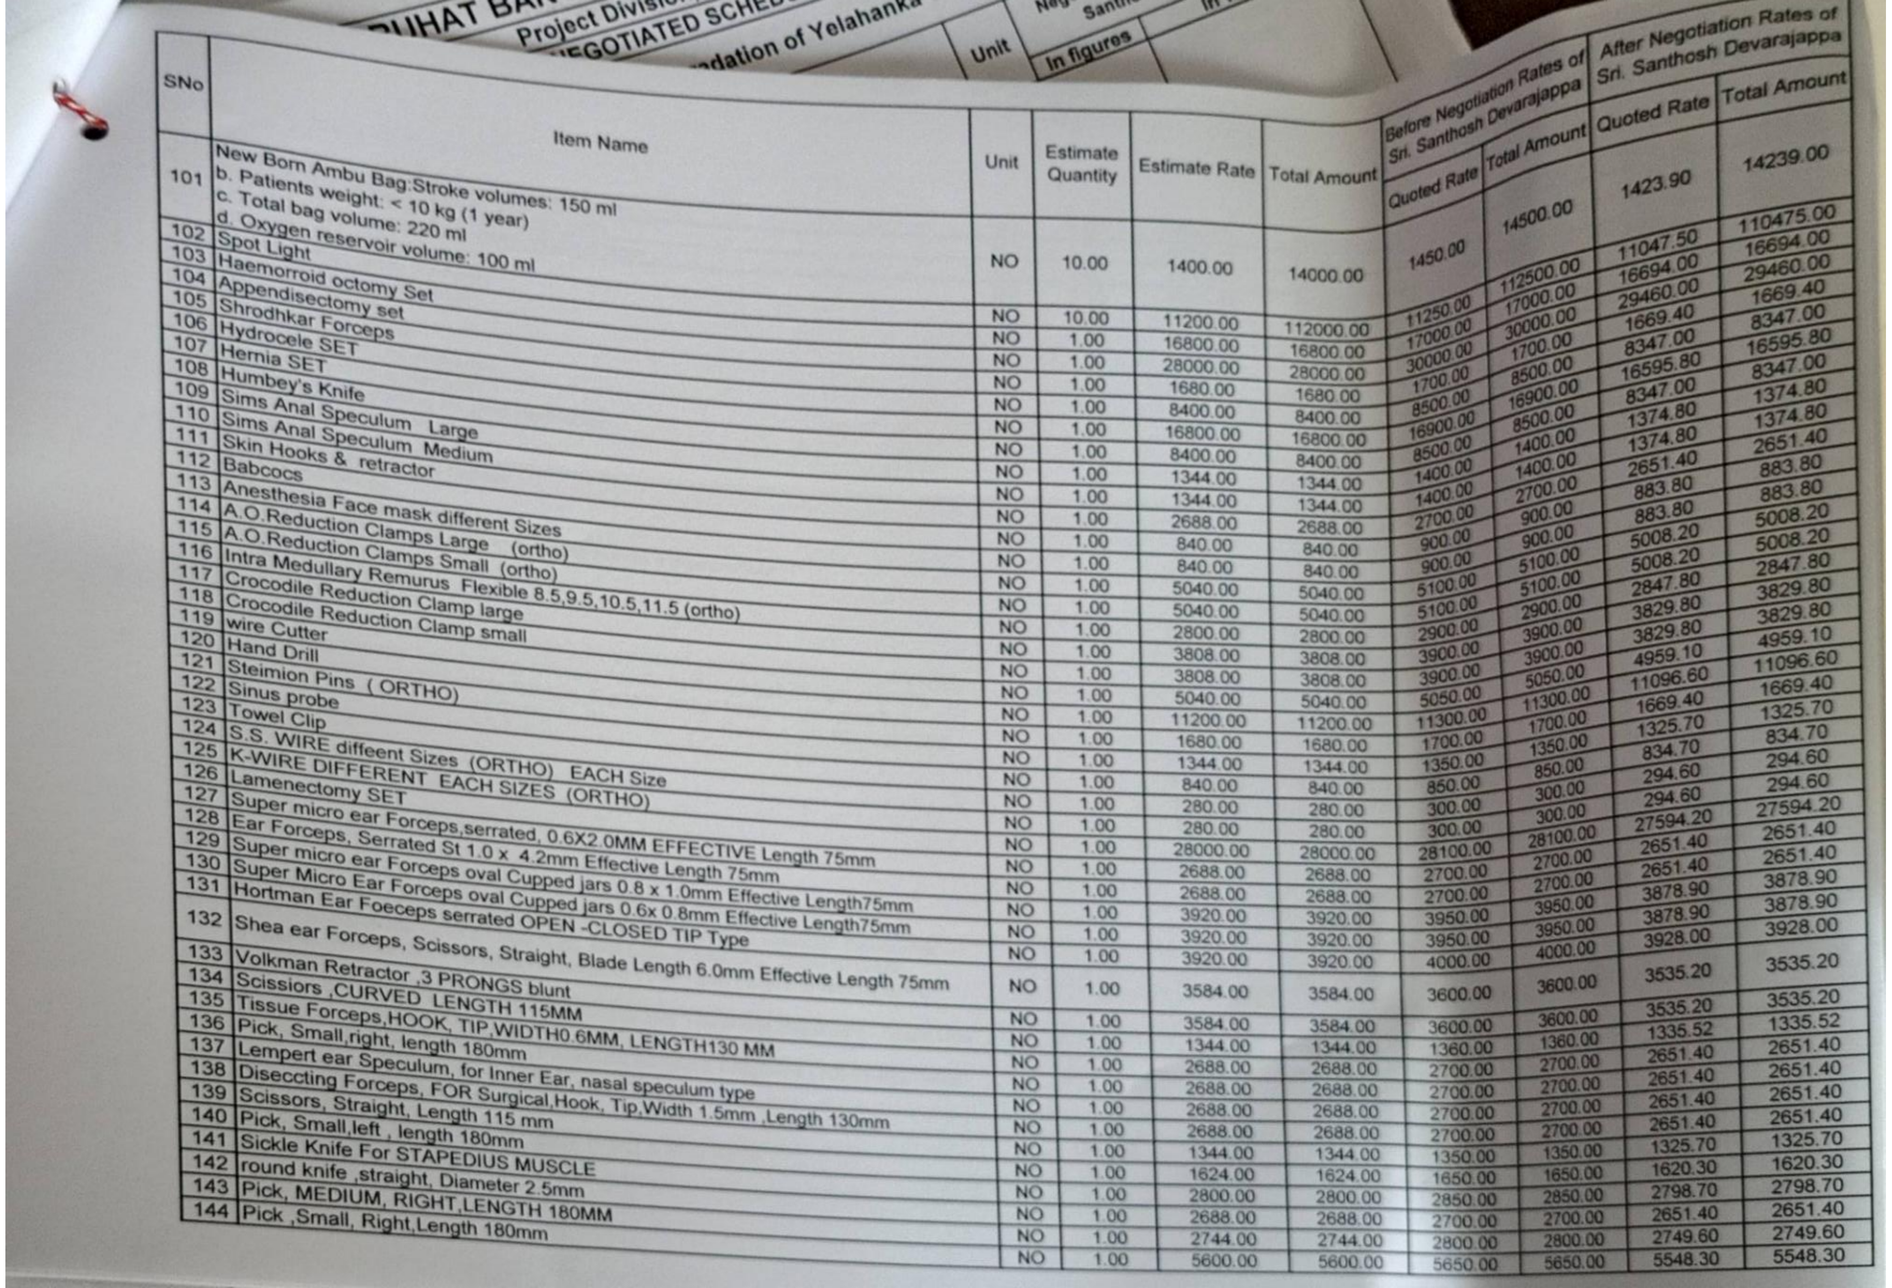

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
101	New Born Ambu Bag:Stroke volumes: 150 ml b. Patients weight: < 10 kg (1 year) c. Total bag volume: 220 ml d. Oxygen reservoir volume: 100 ml	NO	10.00	1400.00	14000.00	1450.00	14500.00	1423.90	14239.00
102	Spot Light	NO	10.00	11200.00	112000.00	11250.00	112500.00	11047.50	110475.00
103	Haemorroid octomy Set	NO	1.00	16800.00	16800.00	17000.00	17000.00	16694.00	16694.00
104	Appendisectomy set	NO	1.00	28000.00	28000.00	30000.00	30000.00	29460.00	29460.00
105	Shrodhkar Forceps	NO	1.00	1680.00	1680.00	1700.00	1700.00	1669.40	1669.40
106	Hydrocele SET	NO	1.00	8400.00	8400.00	8500.00	8500.00	8347.00	8347.00
107	Hernia SET	NO	1.00	16800.00	16800.00	16900.00	16900.00	16595.80	16595.80
108	Humbey's Knife	NO	1.00	8400.00	8400.00	8500.00	8500.00	8347.00	8347.00
109	Sims Anal Speculum Large	NO	1.00	1344.00	1344.00	1400.00	1400.00	1374.80	1374.80
110	Sims Anal Speculum Medium	NO	1.00	1344.00	1344.00	1400.00	1400.00	1374.80	1374.80
111	Skin Hooks & retractor	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
112	Babcocs	NO	1.00	840.00	840.00	900.00	900.00	883.80	883.80
113	Anesthesia Face mask different Sizes	NO	1.00	840.00	840.00	900.00	900.00	883.80	883.80
114	A.O.Reduction Clamps Large (ortho)	NO	1.00	5040.00	5040.00	5100.00	5100.00	5008.20	5008.20
115	A.O.Reduction Clamps Small (ortho)	NO	1.00	5040.00	5040.00	5100.00	5100.00	5008.20	5008.20
116	Intra Medullary Remurus Flexible 8.5,9.5,10.5,11.5 (ortho)	NO	1.00	2800.00	2800.00	2900.00	2900.00	2847.80	2847.80
117	Crocodile Reduction Clamp large	NO	1.00	3808.00	3808.00	3900.00	3900.00	3829.80	3829.80
118	Crocodile Reduction Clamp small	NO	1.00	3808.00	3808.00	3900.00	3900.00	3829.80	3829.80
119	wire Cutter	NO	1.00	5040.00	5040.00	5050.00	5050.00	4959.10	4959.10
120	Hand Drill	NO	1.00	11200.00	11200.00	11300.00	11300.00	11096.60	11096.60
121	Steimion Pins (ORTHO)	NO	1.00	1680.00	1680.00	1700.00	1700.00	1669.40	1669.40
122	Sinus probe	NO	1.00	1344.00	1344.00	1350.00	1350.00	1325.70	1325.70
123	Towel Clip	NO	1.00	840.00	840.00	850.00	850.00	834.70	834.70
124	S.S. WIRE diffeent Sizes (ORTHO) EACH Size	NO	1.00	280.00	280.00	300.00	300.00	294.60	294.60
125	K-WIRE DIFFERENT EACH SIZES (ORTHO)	NO	1.00	280.00	280.00	300.00	300.00	294.60	294.60
126	Lamenectomy SET	NO	1.00	28000.00	28000.00	28100.00	28100.00	27594.20	27594.20
127	Super micro ear Forceps,serrated, 0.6X2.0MM EFFECTIVE Length 75mm	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
128	Ear Forceps, Serrated St 1.0 x 4.2mm Effective Length 75mm	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
129	Super micro ear Forceps oval Cupped jars 0.8 x 1.0mm Effective Length75mm	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
130	Super Micro Ear Forceps oval Cupped jars 0.6x 0.8mm Effective Length75mm	NO	1.00	3920.00	3920.00	3950.00	3950.00	3878.90	3878.90
131	Hortman Ear Foeceps serrated OPEN -CLOSED TIP Type	NO	1.00	3920.00	3920.00	3950.00	3950.00	3878.90	3878.90
132	Shea ear Forceps, Scissors, Straight, Blade Length 6.0mm Effective Length 75mm	NO	1.00	3920.00	3920.00	4000.00	4000.00	3928.00	3928.00
133	Volkman Retractor ,3 PRONGS blunt	NO	1.00	3584.00	3584.00	3600.00	3600.00	3535.20	3535.20
134	Scissiors ,CURVED LENGTH 115MM	NO	1.00	3584.00	3584.00	3600.00	3600.00	3535.20	3535.20
135	Tissue Forceps,HOOK, TIP,WIDTH0.6MM, LENGTH130 MM	NO	1.00	1344.00	1344.00	1360.00	1360.00	1335.52	1335.52
136	Pick, Small,right, length 180mm	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
137	Lempert ear Speculum, for Inner Ear, nasal speculum type	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
138	Diseccting Forceps, FOR Surgical,Hook, Tip,Width 1.5mm ,Length 130mm	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
139	Scissors, Straight, Length 115 mm	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
140	Pick, Small,left , length 180mm	NO	1.00	1344.00	1344.00	1350.00	1350.00	1325.70	1325.70
141	Sickle Knife For STAPEDIUS MUSCLE	NO	1.00	1624.00	1624.00	1650.00	1650.00	1620.30	1620.30
142	round knife ,straight, Diameter 2.5mm	NO	1.00	2800.00	2800.00	2850.00	2850.00	2798.70	2798.70
143	Pick, MEDIUM, RIGHT,LENGTH 180MM	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
144	Pick ,Small, Right,Length 180mm	NO	1.00	2744.00	2744.00	2800.00	2800.00	2749.60	2749.60
		NO	1.00	5600.00	5600.00	5650.00	5650.00	5548.30	5548.30

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
145	Rosen Probe 90 DEGREE ,Tip Length 0.6mm	NO	1.00	5600.00	5600.00	5650.00	5650.00	5548.30	5548.30
146	Rosen Probe 90 DEGREE ,Tip Length 1mm	NO	1.00	5824.00	5824.00	5850.00	5850.00	5744.70	5744.70
147	Lengenbeck periostem Raspatory, Width 6.5mm	NO	1.00	5040.00	5040.00	5100.00	5100.00	5008.20	5008.20
148	Langenbeck periosteal elivator	NO	1.00	5040.00	5040.00	5100.00	5100.00	5008.20	5008.20
149	Wullstein raspiratory ,Curved	NO	1.00	2800.00	2800.00	2850.00	2850.00	2798.70	2798.70
150	Lucae ear Forceps, no hook	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
151	Myringtomy Knife	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
152	Shah's Ear Grommet	NO	1.00	2800.00	2800.00	2800.00	2800.00	2749.60	2749.60
153	Mollison's MASTOID Retractor	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
154	Lempert's Enduaral Retractor	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
155	Jansen's Self Retaining Mastoid Rectractor	NO	1.00	3584.00	3584.00	3600.00	3600.00	3535.20	3535.20
156	Lempert's Endural Speculum	NO	1.00	1680.00	1680.00	1700.00	1700.00	1669.40	1669.40
157	Electric Burrv Mastoid Guage	NO	1.00	1680.00	1680.00	1700.00	1700.00	1669.40	1669.40
158	Macewen currette & cell Seeker	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
159	Crocodile Forceps	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
160	Farabeaf periosteal Elevator	NO	1.00	2240.00	2240.00	2300.00	2300.00	2258.60	2258.60
161	Bur set a) cutting bur, b) cutting diamond bur, c) a diamond bur	NO	1.00	6048.00	6048.00	6100.00	6100.00	5990.20	5990.20
162	Mastoid Drill Piece	NO	1.00	5040.00	5040.00	5100.00	5100.00	5008.20	5008.20
163	Mastoid Drill Machine	NO	1.00	60480.00	60480.00	61000.00	61000.00	59902.00	59902.00
164	Gelform 14 ,Born wax	NO	1.00	16800.00	16800.00	16800.00	16800.00	16497.60	16497.60
165	Cateract set : Corneal Forceps(colubri), conjuncitival scissiors, dialers, lens extractor, suture tying forceps, lens holding forceps, needle holders, small straight scissors, vanna's scissors,capsulorehxis forceps, Superior rectus forceps, Universal Eye Speculum, Anterior Chamber Cannulas (two way), A.C. Needles, Iris REPOSITORS	NO	1.00	16800.00	16800.00	16800.00	16800.00	16497.60	16497.60
166	Chalazion set:	NO	1.00	11760.00	11760.00	11800.00	11800.00	11587.60	11587.60
167	Pterygium Set	NO	1.00	16800.00	16800.00	16800.00	16800.00	16497.60	16497.60
168	Foreign Body Removal Set	NO	1.00	6048.00	6048.00	6100.00	6100.00	5990.20	5990.20
169	Lid retractors	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
170	Lacrymal Syringing Needle/	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
171	Lacrymal Probe	NO	1.00	1680.00	1680.00	1700.00	1700.00	1669.40	1669.40
172	Punctum Dialtor	NO	1.00	2688.00	2688.00	2700.00	2700.00	2651.40	2651.40
173	Panasinc NS300 IP EPABX, PANASONIC KEY TELEPHONE SYSTEM - NS300,Configured for 6 trunk Lines ,2 digital extention & 60 analouge Extensions, Further Expandable up to 8 Lines & 96 analouge Extensions. Caller ID option Available. Built in SMDR & USB Port.Built in Voice DISA (Greeting Message).PC Programmable	NO	1.00	161660.00	161660.00	165000.00	165000.00	162030.00	162030.00
174	KEY TELEPHONE INSTRUMENT:Panasonic Key Telephone instrument - Single Line Display,12 Programmable Keys,High Quality Speaker Phone	NO	1.00	10502.00	10502.00	10600.00	10600.00	10409.20	10409.20
175	TELEPHONE INSTRUMENTS - Panasonic Standard Telephone - KX-TS400,Timed Flash,3 Step Ringer Selector ,Wall Mountable	NO	60.00	767.00	46020.00	800.00	48000.00	785.60	47136.00
176	MDF 20 Pair with MDF BOX	NO	4.00	3245.00	12980.00	3300.00	13200.00	3240.60	12962.40
177	CAT 6 Cable	M	1200.00	30.68	36816.00	40.00	48000.00	39.28	47136.00
178	R. O. Plant (For Major OT and Labour Ward) & other wards	NO	8.00	21240.00	169920.00	21500.00	172000.00	21113.00	168904.00
179	Fire Extinguishers Type A, B, C (6KGS)	NO	20.00	2478.00	49560.00	2550.00	51000.00	2504.10	50082.00

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
180	DIALYSIS : A. General 1. The machine should be capable of doing all the following renal replacement treatment as mentioned below a. Haemodialysis (Normal HD) b. Online Hemodiafiltration c. Online Hemofiltration d. SLED (sustained low efficiency Dialysis) e. Sustained low-efficiency daily diafiltration SLEDDF f. Extended daily diafiltration EDD-f g. Prolonged daily intermittent renal replacement therapy (PDIRRT) h. Go-slow dialysis i. Hybrid renal replacement modalities 2. The machine should have two roller pumps. One is for blood pump; other is substitution pump for generating replacement fluid which is used during online modiafiltration and online Hemofiltration therapies. 3. Blood pump – blood flow range should be (effective) 30 to 600 m/min, accuracy ± 10% 4. Effective blood flow rate should be calculated and displayed on the front panel in a real time basis during dialysis automatically 5. It shall be easy and safe to thread with bloodline diameter from 2 mm up to 10 mm 6. Automatic set up and priming is preferred 7. An emergency hand crank shall be provided for returning blood to patient when electrical power is lost. Direction of rotation shall be limited or visually indicated 8. Single needle system 2 blood pumps, internal pressure/pressure control with variable stroke volume(max 50 ml) 9. Dialysate flow: a. Dialysis fluid flow range should be selectable from 0-1000 ml/min (steps of 100 ml/min) 10. Dialysate flow should be on adequacy favoured basis 11. Auto flow (selectable) automatic adaption of the dialysate flow to the effective blood flow (factors adjustable) 12. Dialysate consumption basis (It should be on selectable mode on needed basis) B. Substitute Flow 1. Substitution fluid should be generated by machine itself from the hydraulic by filtering the dialysate through 2 endotoxin filters in series 2. Auto sub: where the machine can select optimum substitute flow according to the treatment condition. Auto sub substitution method should ideally match to effective	NO	2.00	1475000.00	2950000.00	1576038.00	3152076.00	1547669.32	3095338.63
181	Solar water - 500 lpd ETC SWH (PC) 58 dia	NO	4.00	45150.00	180600.00	46000.00	184000.00	45172.00	180688.00
182	SOLAR WATER -PLUMBING	LS	1.00	149270.00	149270.00	150000.00	150000.00	147300.00	147300.00
183	High Definition Projector: Projector WXGA, 3600Lumens	NO	2.00	56320.00	112640.00	57000.00	114000.00	55974.00	111948.00
184	Tripod For Projector :Ceiling Mount	NO	2.00	3540.00	7080.00	3600.00	7200.00	3535.20	7070.40
185	Tripod For Screen: Logic7x5 pull down screen,	NO	2.00	8850.00	17700.00	9000.00	18000.00	8838.00	17676.00
186	Loud Speaker :Honeywell Ceiling Speaker 6W,8ohm	NO	5.00	1416.00	7080.00	1500.00	7500.00	1473.00	7365.00
187	Cordless Mike: MX/Studio Master	NO	5.00	12160.00	60800.00	12200.00	61000.00	11980.40	59902.00
188	Computer: High Configuration, 2TB Ram, Generation Core i 7/i 9, :HP EliteDesk 800 G4 MT ⊘i7-8700-8GB DDR4 RAM, AMD Radeon R7 430 2GB Gfx Dedicated2TB HDD with 7200 RPM, DOS, DVD RW, 18.5" TFT, 3 yearson site warranty	NO	25.00	88500.00	2212500.00	94562.00	2364050.00	92859.88	2321497.10
189	Jumbo Jet zerox Machine (1 COLOURED)-HP LASERJET 1136 MFP PRINTER -ALL-IN -ONE Print,scan,copy	NO	2.00	17464.00	34928.00	18000.00	36000.00	17676.00	35352.00
190	Printer with Scanner(COLOURED) (A4)-Speed: 25 PPM(Network Printing, Copying,Scanning & Wifi)A4 Size –Pass 600x600 DPI Document Feeder)Scan to mail, Scan to folde(UFR II Fast Rendering IIDirect Print From USB Pen Drive	NO	25.00	18290.00	457250.00	19543.00	488575.00	19191.23	479780.65

Patient Cots (Plain):1. Size-... 2. The head bow and leg ... Head and leg bows ERW Tube.2. The head bow and leg ... Head and leg bows are 14 gauge, 1" dia ERW ... Rupees Six ...

Scanned by TapScanner

SNo	Item Name	Unit	Estimate Quantity	Estimate Rate	Total Amount	Before Negotiation Rates of Sri. Santhosh Devarajappa		After Negotiation Rates of Sri. Santhosh Devarajappa	
						Quoted Rate	Total Amount	Quoted Rate	Total Amount
191	52" Monitor LED With Cameras (high Resolution) with Security Alert with backup UPS Systems -Panasoniv Monitor55" LED Monitor	NO	15.00	76700.00	1150500.00	81954.00	1229310.00	80478.83	1207182.42
192	Pen Drive 128 GB-SANDISC128 gb pen drive	NO	10.00	2360.00	23600.00	2400.00	24000.00	2356.80	23568.00
193	Hard Disc 1TB-Segate HDD 1 TB EXTERNAL Back up hdd	NO	10.00	10620.00	106200.00	11000.00	110000.00	10802.00	108020.00
194	32" Colour Television-32" TV Panasonic	NO	5.00	16000.00	80000.00	16000.00	80000.00	15712.00	78560.00
195	online UPS FOR COMPUTERS ALL COMPUTERS	NO	25.00	4130.00	103250.00	4150.00	103750.00	4075.30	101882.50
196	Computers Acessories (wire less key board, Mouse)-HP Wireless KB & MOUSE	NO	20.00	1534.00	30680.00	1550.00	31000.00	1522.10	30442.00
197	Lap Top-HP i5-8250U, 4GB DDR4 RAM, 1TB SATA14" LED HD, No DVDRW, 1 Yr Onsite Warranty with 1Yr ADP, With Bag	NO	2.00	60180.00	120360.00	65000.00	130000.00	63830.00	127660.00
198	Camera DSLR (meeting /program) :Nikon DSLR	NO	2.00	39530.00	79060.00	41000.00	82000.00	40262.00	80524.00
199	labomed binacular microscope with UPS BACK UP (180-250V /ac):Viewing Body: Bino/Trino Butterfly style Adjestable height 30deg, incline, 360 rotable Single Mould stand with Extended base for hand rest. Reverse quadruple nose piece. Ultra Smooth Cam technology Co-axail controls Coarse & Fine focus knob. RACKLESS Double plate stage with Co-axail control for x/y movement of slide, DOUBLE Slide holder.Illumination: 6v-20w HALOGEN bulb OR LED with built-in battery Back of approx. 2 Hrs, with intensity control. the system allows flate field image and superb contrast in expanded 20mm field of view.Obj.: infinity PLAN Ach. 4x,10x,40, (SL), 100x(SL) Oil Imm. Eye Piece : WF 10x (FOV 20), Focusable with eye guards.	NO	1.00	84960.00	84960.00	90000.00	90000.00	88380.00	88380.00
200	Harmone Analyser :Feature : • Throughput: up to 180 tests/hour • 24 hours ready-to-use • Time to first result:17 minutePrinciple of Luminescence • Non-enzyme involved flash chemiluminescence, long stability of reagents • ABEI label, stable in acid and alkaline solution Modes of Operation • Random, Batch and STAT Sample Loading • Up to 16 sample tubes • Continuous loading, STAT available • Analyzer auto numbered • LIS connection • Refrigerated sample area with independent power supply Reagent Loading • 4 reagents on board • Continuous loading • RFID reading all info of reagents • Refrigerated reagent area Reagent Features • Integrated kit, ready-to-use, no pretreatment required • Integrated kit including calibrators • Using superparamagnetic microbeads • RFID tag storing all info of reagent • RFID tag with built-in master curve • 2-point calibration to adjust master curve • Calibration stability: Max 4 weeks Other Features • Clot detection • Liquid level detection for reagent • Optional ratio for sample dilutionAuto dilution for high concentration sample • Constant 37℃ incubation • 15-30℃ Operating Temperature Operation System • Windows 7 • HP compatible (Dual-core CPU), Color touch screen Interconnection • Connection to	NO	1.00	1003000.00	1003000.00	1071706.00	1071706.00	1052415.29	1052415.29
201	Protein Analyser Including HBA1C:TECHNICAL CHARACTERISTICS Autonomy , Continuous sample loadingTube capacity Proteins: 28 samplesHbA1c, Hb or CDT: 26 samplesThroughput Proteins: 20 tests/h HbA1c or Hb: 7 tests/hCDT: 10 tests/h Sample types Serum,Whole blood (capped tubes)Positive ID & Reagents TraceabilityBarcoded carousel and tubesHigh resolution built-in barcode readerPositive sample identificationFull traceability from primary tube to final resultBarcoded reagents and controls Sampling modeFull automation with continuous loadingDirect sampling from primary tubesSampling from open and capped tubes (cap piercing)Efficient mixing system with multiple sample inversionsCapillaries2 silica capillaries for 2 simultaneous migrations Migrations performed in capillaries at accurate temperature controlled by a Sebia proprietary Peltier based regulation device	NO	1.00	2183000.00	2183000.00	2332536.00	2332536.00	2290550.35	2290550.35

Patient Cots (Plain... 20

Scanned by TapScanner